

# Natural Allergy Method Radionics Chart

6 Dixon Street Wangaratta Victoria 3677 | 03 5798 3344 | myhealth@nenaturopathicgroup.com.au

---


## MASTER MODULE M4 MANUAL

- 1, 2) Card slots 1 and 2; insert cards here, the rings must face you for all potencies except LM potencies.  
Avoid cards with more than eight sector marks. When using slot 1, set switch 11 to CARD position.
- 3) RECIPIENT vessel; place the medium to be potentised into or over this well, use only cylindrical containers.
- 4) SOURCE plate; deposit any physical matter here to make a nosode. Set switch 11 to plate for this function. Please note the model M4, unlike other instruments, does not alter the potency of the original.
- 5) OUTPUT; this socket has the same potential as the RECIPIENT well. It can be used to produce large quantities of remedies or to make a remedy bath. Insert the white plug of the external output cable here.
- 6) EXTENDER socket; insert the plug of an EXTENDER MODULE E4 here, if you want to expand to more slots.  
Be sure to have unused channels switched off to prevent accidental neutralisation of remedies!
- 7) Precision potentiometer; set to required potency code for channel 2. See Potency Code List for M3P, M4
- 7a), 8a) Locking brake in free position; push left to lock potentiometer after code setting.
- 8) Precision potentiometer; set to required potency code for channel 1. see potency code list  
Then choose CARD or PLATE with switch 11.
- 9) CHANNEL switch for card slot 2; to prevent accidental neutralisation of remedies made in channel 1, switch to OFF while not in use.
- 10) CHANNEL switch for card slot 1 card or plate; to prevent accidental neutralisation of remedies made in channel 2, switch to OFF while not in use.
- 11) Selector switch; choose between CARD or PLATE, when using channel 1.

Please note, when setting potency dials to 10 MM = 1000. The dial has for economic reasons only 3 digits, the number 1 of 1000 is not visible. After 999, the next position 000 equals 1000 this would be close to the fully clockwise end position.

**To comply with the Australian Therapeutic Goods Act 1990 the manufacturer recommends:**

- A) Using this instrument only to make homoeopathic remedies above 4X on a one to one basis by certified homeopaths for extemporaneous prescribing, exempt in research applications.
- B) Ensuring that remedies contain sufficient alcohol to prevent growth of micro organisms.

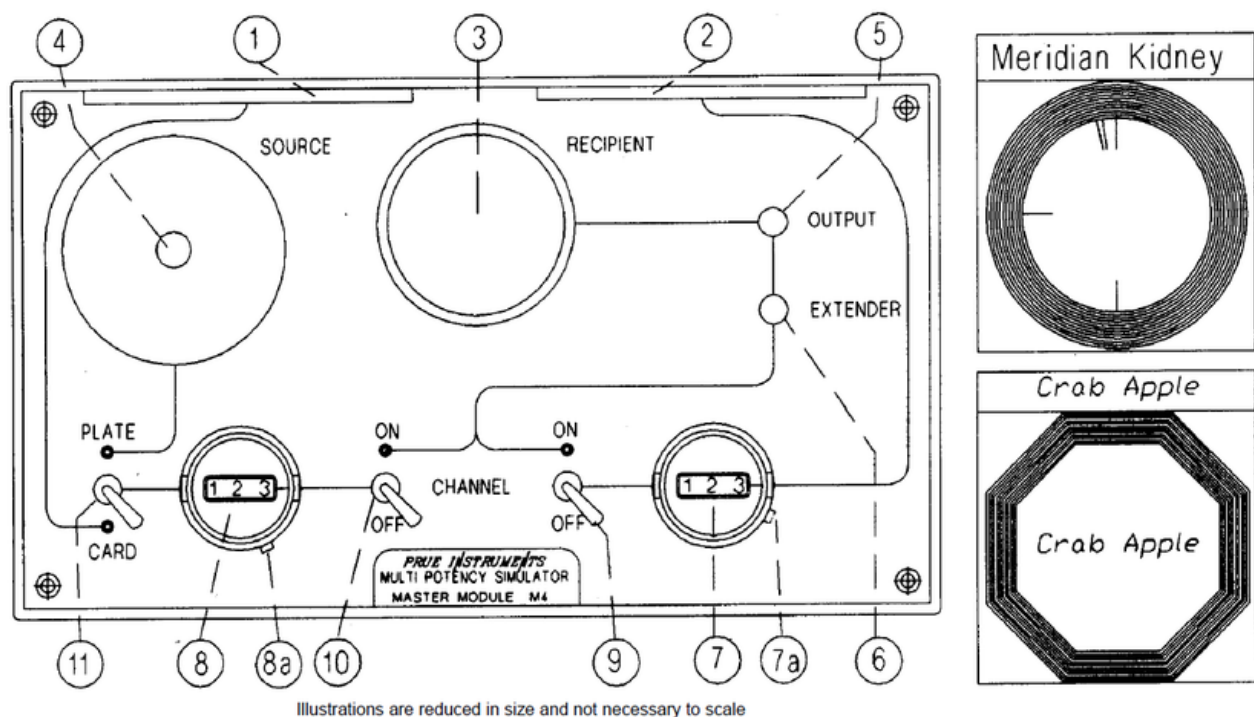

M4info.pub 091220

## TO MAKE A POTENCY FROM ONE OR MORE CARDS.

Insert a clean round bottle filled with the medium, distilled water \ alcohol mix into the recipient well or directly above it.

Switch on only the desired number of channels and set the selected potencies codes. See Potency Code List for M4.

Insert the cards in the appropriate slots with the concentric rings or octagons facing you.

This order is chosen to give the instrument a chance to wipe any randomly existing potencies from bottle or contents.

The exposure time is 3 minutes for water \ alcohol mix and 5 minutes for moistened milk sugar or saclac pilules. Longer exposure is not of any benefit as it takes only 3 minutes to rearrange water molecules to form liquid crystals.

Remove the potentised medium from the well first, or all channels must be switched to off, before any cards are removed. If this rule is not followed, the instrument will erase all potencies before you can get the bottle out of the well.

## **TO MAKE A POTENCY FROM ANY PHYSICAL SUBSTANCE OR COPY A REMEDY.**

A finger print, or a bit of dust, on the stainless steel source plate will produce a remedy ! Clean it with a clean tissue, distilled water \ alcohol mix and, if needed, silver polish can be used, first.

Place a clean round bottle containing a suitable medium in the recipient well.

Switch channel 1 to on and the selector switch to plate, then dial the selected potency code. See Potency Code List.

It is possible to copy remedies up and down, you can make a 10MM from 6X as well as a 6X from a 10MM source.

Place a drop, pill, a bottle of tincture, remedy or item that you want to make a different potency or remedy from on the source plate. Select the desired Potency code from the Potency Code list and dial the code on Potentiometer (8).

Exposure time is 3 minutes for liquids and 5 minutes for moistened milk sugar or saclac pilules.

Take the potentised medium from the well first, or the channel must be switched to off before the source is removed. If this rule is not followed, the instrument will erase the potency before you can get the bottle out of the well.

The M4 model does not alter the potency of the source as some other instruments do. Dispose of or remove the sample from the source plate and clean it thoroughly.

Multiple potency remedies can be copied, but the result does not reproduce the various multiple potencies of the original ! You will end up with one potency for all according to the setting of the potentiometer.

## **RESEARCH APPLICATION ONLY:**

It is possible to project the information from a card in the slot and \ or an item on the source plate to the energy field (aura) of any person, animal or piece of land of your choice located anywhere on this planet.

I recommend that you try this work on yourself first, or with someone close by, so that its progress can be easily monitored and recorded carefully before you experiment with someone else at long distance. Bear in your mind that you treat a whole person or pet not only a single organ or disease, Bach- or Bush- flower remedies are very suitable for this procedure.

You need to have:

A signed request of the person in need. Every person has the right to suffer and learn the lesson to be learned, we are not allowed to take this privilege away.

- The skill to select a remedy and the correct potency with the pendulum.
- The skill to select the time span of projection (this can vary between seconds and several days).

- The skill to select the time to start. (The person could be driving while you give a sedating projection).
- It is your responsibility to ensure that projection times are not extended
- The implications can be disastrous. SET A RELIABLE ALARM CLOCK !!

Use the outer rim of the provided sector chart that gives you a 0 to 100 % scale and search for the % of life force left and write it down.

After inserting the selected card and dialling the required potency, simply place the signature, hair, sputum, sweat or urine sample in the recipient well instead of a medium bottle.

Please note that the sequence is different, as you do not desire to neutralise the person or pet. Put the sample or witness in last and take it out first from the well at the end of projection. At the end of projection check the life force % of the patient and see if you can improve this situation further by projecting another remedy.

The manufacturer reserves the right to change design and specifications without notice in order to improve this instrument.

M4info.pub 091220

# Natural Allergy Method Radionics Chart

6 Dixon Street Wangaratta Victoria 3677 | 03 5798 3344 | myhealth@nenaturopathicgroup.com.au

## Potency Code List for M3P, M4 Master and Extender Modules

|            |                           |                       |                         |
|------------|---------------------------|-----------------------|-------------------------|
| 1 X--- 60  | 1 C --269                 | 1 M-- 582             | 1 MM-- 895              |
| 2 X--- 92  | 2 C --300                 | 2 M-- 613             | 2 MM-- 926              |
| 3 X-- 110  | 3 C --319                 | 3 M-- 632             | 3 MM-- 945              |
| 4 X-- 123  | 4 C --332                 | 4 M-- 645             | 4 MM-- 958              |
| 5 X-- 133  | 5 C --342                 | 5 M-- 655             | 5 MM-- 968              |
| 6 X-- 141  | 6 C --350                 | 6 M-- 663             | 6 MM-- 976              |
| 7 X-- 148  | 7 C --357                 | 7 M-- 670             | 7 MM-- 983              |
| 8 X-- 154  | 8 C --363                 | 8 M-- 676             | 8 MM-- 989              |
| 9 X-- 160  | 9 C --368                 | 9 M-- 681             | 9 MM-- 994              |
| 10 X-- 165 | 10 C --373                | 10 M-- 686            | 10 MM--1000             |
| 11 X-- 169 | 11 C --378                | 11 M-- 690            |                         |
| 12 X-- 173 | 12 C --381                | 12 M-- 694            | EXPOSURE TIME FOR       |
| 13 X-- 176 | 13 C --385                | 13 M-- 698            | POTENCIES               |
| 14 X-- 180 | 14 C --388                | 14 M-- 701            | 1X TO 10 MM             |
| 15 X-- 183 | 15 C --392                | 15 M-- 705            | For water alcohol mix:  |
| 16 X-- 186 | 16 C --395                | 16 M-- 707            | 3 minutes.              |
| 17 X-- 189 | 17 C --397                | 17 M-- 710            |                         |
| 18 X-- 191 | 18 C --400                | 18 M-- 713            | For milk sugar powder   |
| 19 X-- 194 | 19 C --402                | 19 M-- 715            | or pilules:             |
| 20 X-- 196 | 20 C --405                | 20 M-- 718            | 5 to 10 minutes         |
| 21 X-- 198 | 25 C --415                | 25 M-- 730            | depending on the        |
| 22 X-- 200 | 30 C --423                | 30 M-- 736            | moisture content.       |
| 23 X-- 202 | 35 C --430                | 35 M-- 744            |                         |
| 24 X-- 204 | 40 C --436                | 40 M-- 749            |                         |
| 25 X-- 206 | 50 C --446                | 50 M-- 759            | <b>To make LM</b>       |
| 26 X-- 208 | 60 C --454                | 60 M-- 767            | <b>potencies</b>        |
| 27 X-- 210 | 70 C --461                | 70 M-- 774            | have a stopwatch        |
| 28 X-- 211 | 80 C --467                | 80 M-- 780            | handy.                  |
| 29 X-- 213 | 90 C --473                | 90 M-- 786            | Place remedy bottle     |
| 30 X-- 214 | 100 C --478               | 100 M-- 790           | into                    |
| 31 X-- 216 | 200 C --509               | 200 M-- 822           | the well. Insert a card |
| 32 X-- 217 | 300 C --527               | 300 M-- 840           | into                    |
| 33 X-- 219 | 400 C --540               | 400 M-- 853           | the slot, with the      |
| 34 X-- 220 | 500 C --550               | 500 M-- 863           | rings                   |
| 35 X-- 221 | 600 C --559               | 600 M-- 872           | facing away from you,   |
| 36 X-- 223 | 700 C --566               | 700 M-- 879           | and switch the          |
| 37 X-- 224 | 800 C --572               | 800 M-- 885           | channel                 |
| 38 X-- 225 | 900 C --577               | 900 M-- 890           | switch to on.           |
| 39 X-- 226 |                           |                       |                         |
| 40 X-- 227 | <b>Please note,</b>       | <b>D = X</b>          | Turn the                |
| 42 X-- 230 | When setting the          | <b>D6= 6X</b>         | potentiometer           |
| 44 X-- 232 | potency dial to           |                       | dial from 0 to 10 MM    |
| 46 X-- 234 | 10 MM = 1000.             | <b>CM= 100M</b>       | =0 to 1000, Fully       |
| 48 X-- 236 | The dial has for          | <b>DM= 500M</b>       | clockwise               |
| 50 X-- 238 | economic reasons          |                       |                         |
| 55 X-- 242 | only 3                    | <b>To neutralise</b>  | Exposure time now       |
| 60 X-- 246 | digits, the first digit 1 | remaining             | determines the LM       |
| 65 X-- 249 | of                        | potencies, put item   | potency                 |
| 70 X-- 253 | 1000 is not visible.      | or                    | 1 LM = 1 minutes        |
| 75 X-- 256 | After 999, the next       | bottle into or over   | 2 LM = 2 minutes        |
| 80 X-- 259 | position 000 equals       | the well              | 3 LM = 3 minutes        |
| 85 X-- 262 | 1000                      | and then without a    | .....And so on.         |
| 90 X-- 264 | this is on the fully      | card                  |                         |
|            | clockwise end             | in the slot turn on a |                         |
|            | position.                 | channel switch for a  |                         |
|            |                           | few                   |                         |
|            |                           | seconds. This way     |                         |
|            |                           | you                   |                         |
|            |                           | can re-use bottles    |                         |
|            |                           | and                   |                         |
|            |                           | remedies.             |                         |